

# System Requirements

---

- 1GHz or higher CPU
- 1GB or more RAM
- Hard disk with 2GB or more spare space
- USB 2.0/3.0

## The software supports the following operating systems:

- Microsoft Windows Vista
- Microsoft Windows 7
- Microsoft Windows 8
- Microsoft Windows 10

*If the operating system is lower than the above version, please update the system first.*


## Installation

---

1. Insert the installation CD into the CD-ROM of a computer.
2. The installation interface pops up. (If no installation interface appears, double-click Setup.exe in the CD-ROM directory to start it manually.)

# Using the Software

## 1. Interface

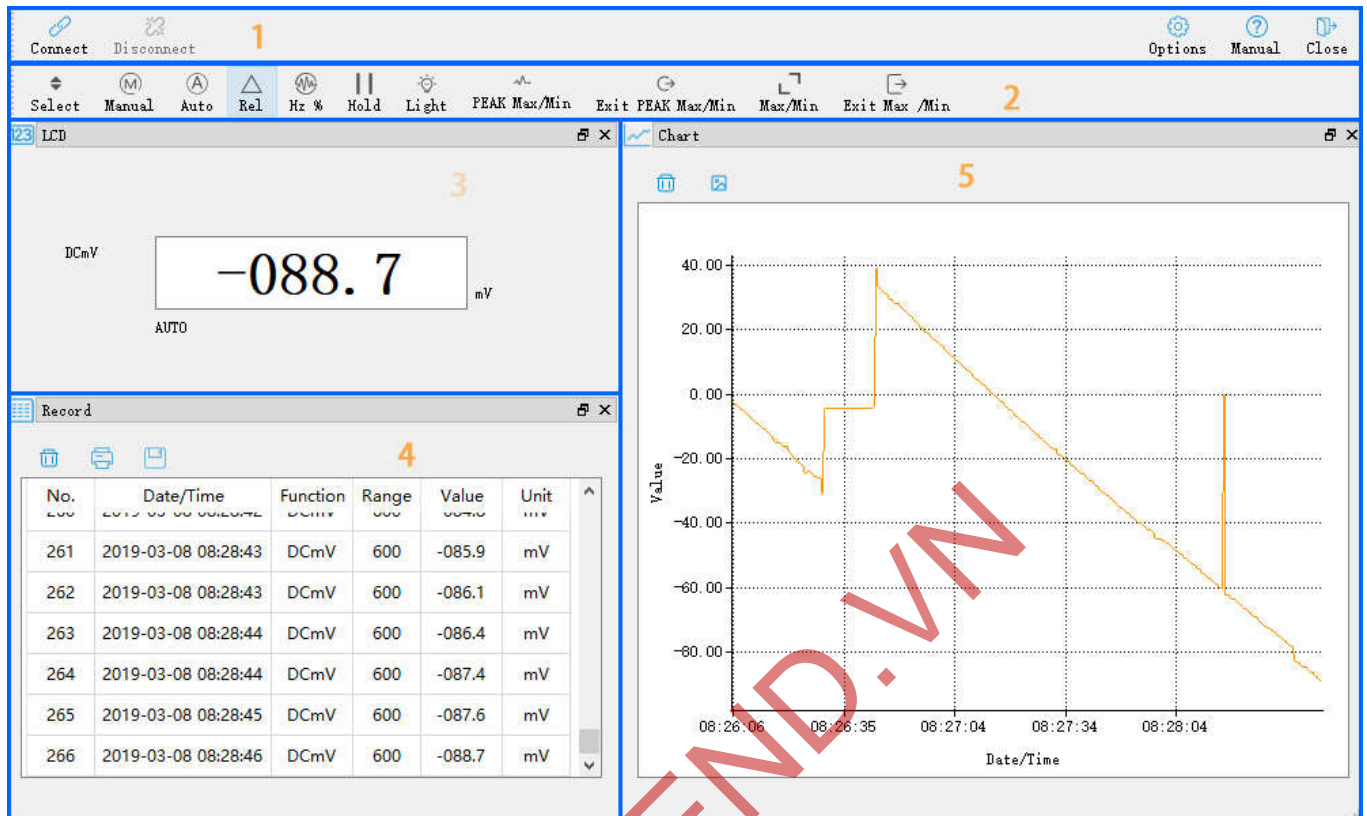

Area	Description
1	Toolbar
2	Control commands
3	Real-time measurement
4	Data records
5	Data chart

## 2. Connect device



- Click **Connect** to connect the device.
- If the connection is successful, the measurement data will be displayed in Area3, Area4 and Area 5.


## 3. Disconnect device




- Click **Disconnect** to disconnect the device.

- Each area will stop displaying measurement data

## 4. Export


- Click  to export the data record to an Excel file

## 5. Clear data

- Click  to clear the recorded data.

## 6. Setup software

- Click  to open options dialog

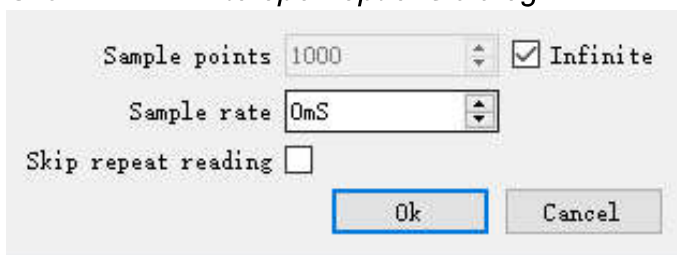

Sample points 1000  Infinite

Sample rate 0mS

Skip repeat reading


Ok Cancel

- “Sample Points”: Set the number of sampling points. If “Infinite” is checked, the number is unlimited
- “Sample rate”: Set the sampling rate. If the set rate is greater than the actual rate, the actual rate will prevail; if set to 0, the actual rate will be sampled
- “Skip repeat reading”: If checked, the same sample value as the previous one is not recorded

## 7. Get help

- Click  to open the “Software user manual”

## 8. Close the software

- Click  to close the software